

On-X Valve MRI Compatibility

MR Conditional  by non-clinical testing*

Static Magnetic Field


- Static magnetic field of 3-Tesla or less
- Maximum spatial gradient magnetic field of 720-Gauss/cm or less

MRI-related Heating

- Highest temperature change = +1.6°C

Artifact Information

- MR image quality may be compromised if the area of interest is in the exact same area or relatively close to the position of the On-X valve.

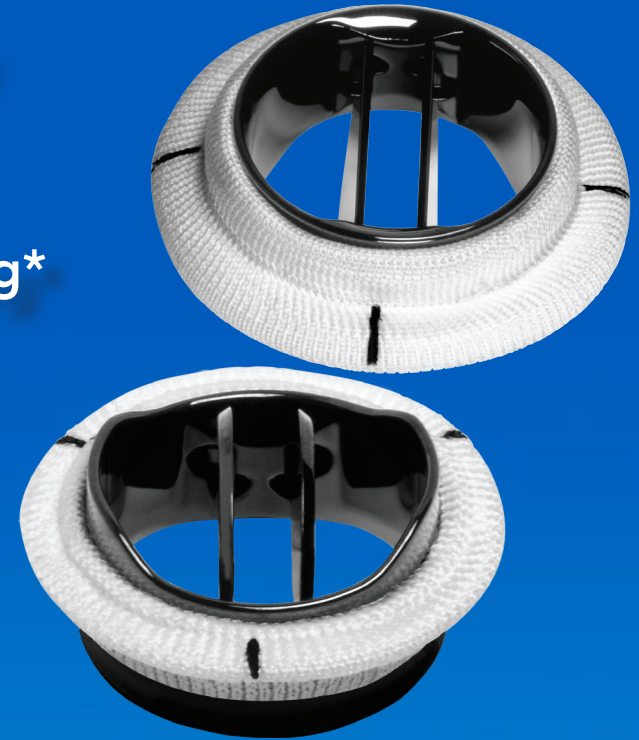

*Further information provided upon request.